
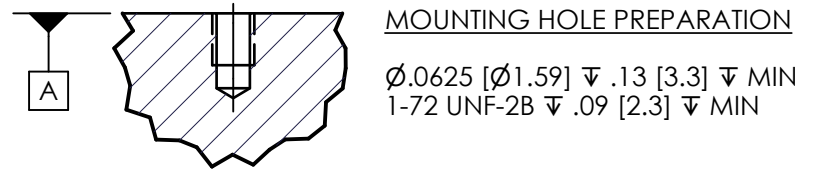
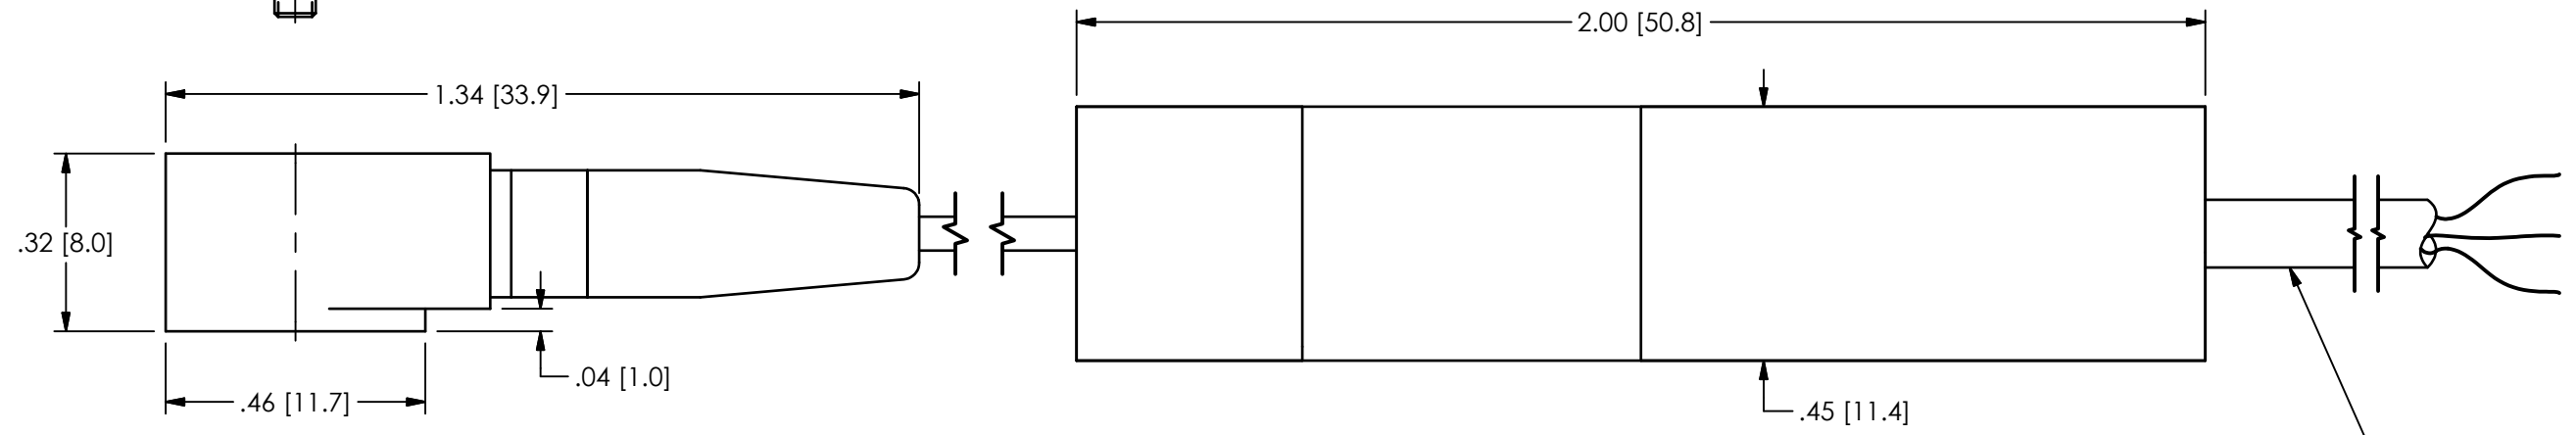
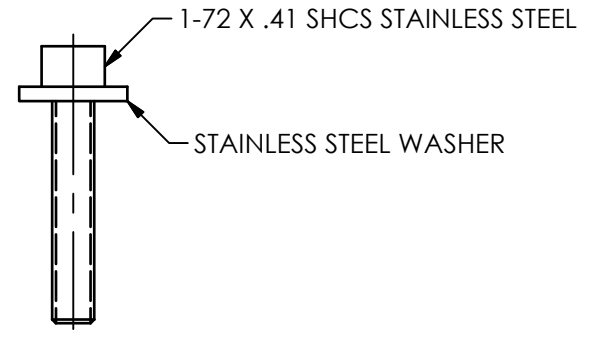


37637

PCB Piezotronics Inc. claims proprietary rights in the information disclosed hereon. Neither it nor any reproduction thereof will be disclosed to others without the written consent of PCB Piezotronics Inc.

REVISIONS		
REV	DESCRIPTION	DIN
C	REVERT TO REV A CABLE	44487

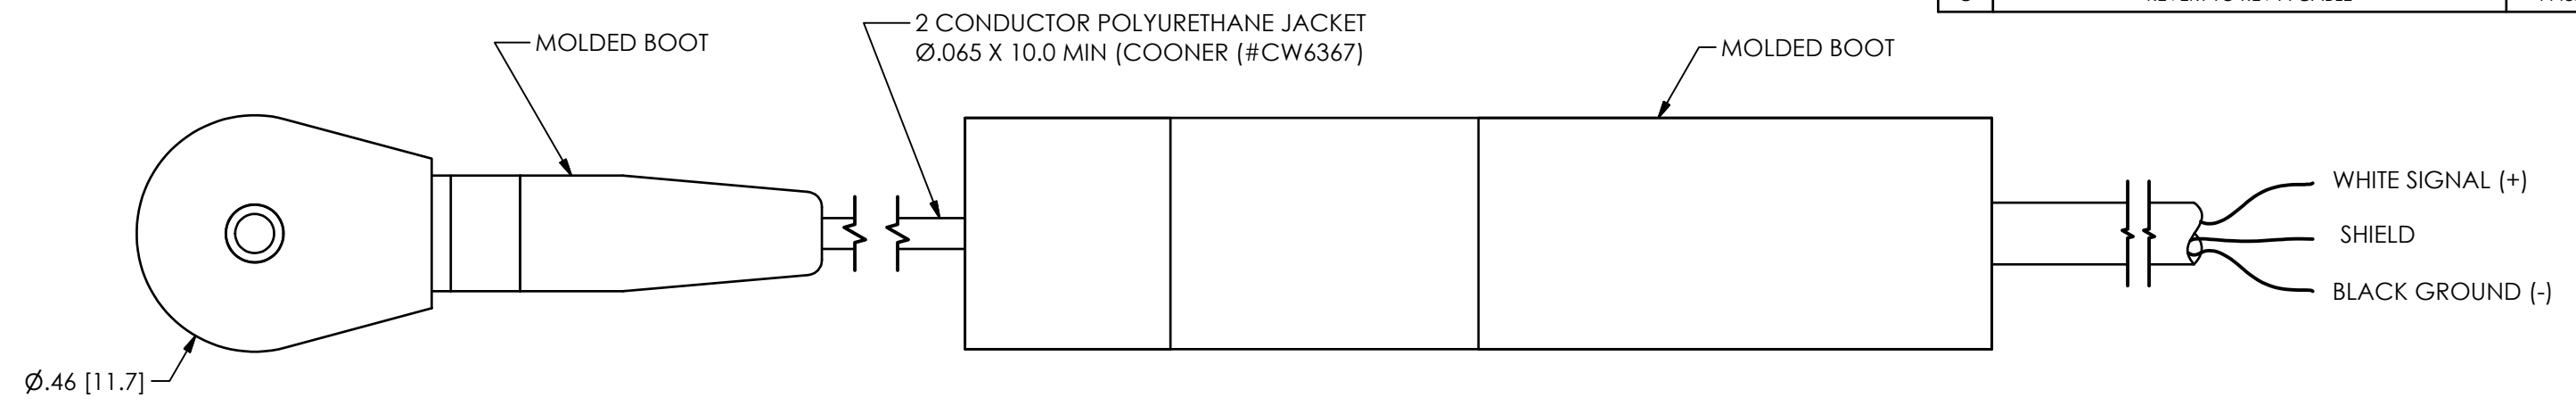

2 CONDUCTOR POLYURETHANE JACKET Ø.156 X 20 FEET TERMINATING IN PIGTAILS (SOUTHBAY #SB-38113)

- 3.) RECOMMENDED MOUNTING TORQUE 1 TO 2 IN-LBS [11 TO 23 N-cm]
- 2.) MOUNTING SURFACE SHOULD BE FLAT TO WITH .001 [0.03] TIR OVER Ø.75 [Ø19.1] WITH A MINIMUM $\sqrt[63]{1.6}$ FOR BEST RESULTS.
- 1.) DRILL PERPENDICULAR TO DATUM "A" TO WITHIN ± 1'.

UNLESS OTHERWISE SPECIFIED TOLERANCES ARE:		DRAWN		CHECKED		ENGINEER	
DIMENSIONS IN INCHES	DIMENSIONS IN MILLIMETERS [IN BRACKETS]	BB	8/28/15	ECB	8/28/15	MAM	8/28/15
DECIMALS XX ±.01 XXX ±.005	DECIMALS X ±.03 XX ±.013	TITLE INSTALLATION DRAWING MODEL 355M73 RING ACCELEROMETER					
ANGLES ± 2 DEGREES	ANGLES ± 2 DEGREES						
FILLETS AND RADII .003 - .005	FILLETS AND RADII 0.07 - 0.13	CODE IDENT. NO. 52681		DWG. NO. 37637		SCALE: 3X SHEET 1 OF 1	

PCB PIEZOTRONICS™
3425 WALDEN AVE. DEPEW, NY 14043
(716) 684-0001 E-MAIL: sales@pcb.com